


# 1) How can I synchronize my spectra with laser firing using TTL signal or analog signal?

Please select Options from the toolbar. (See below picture).

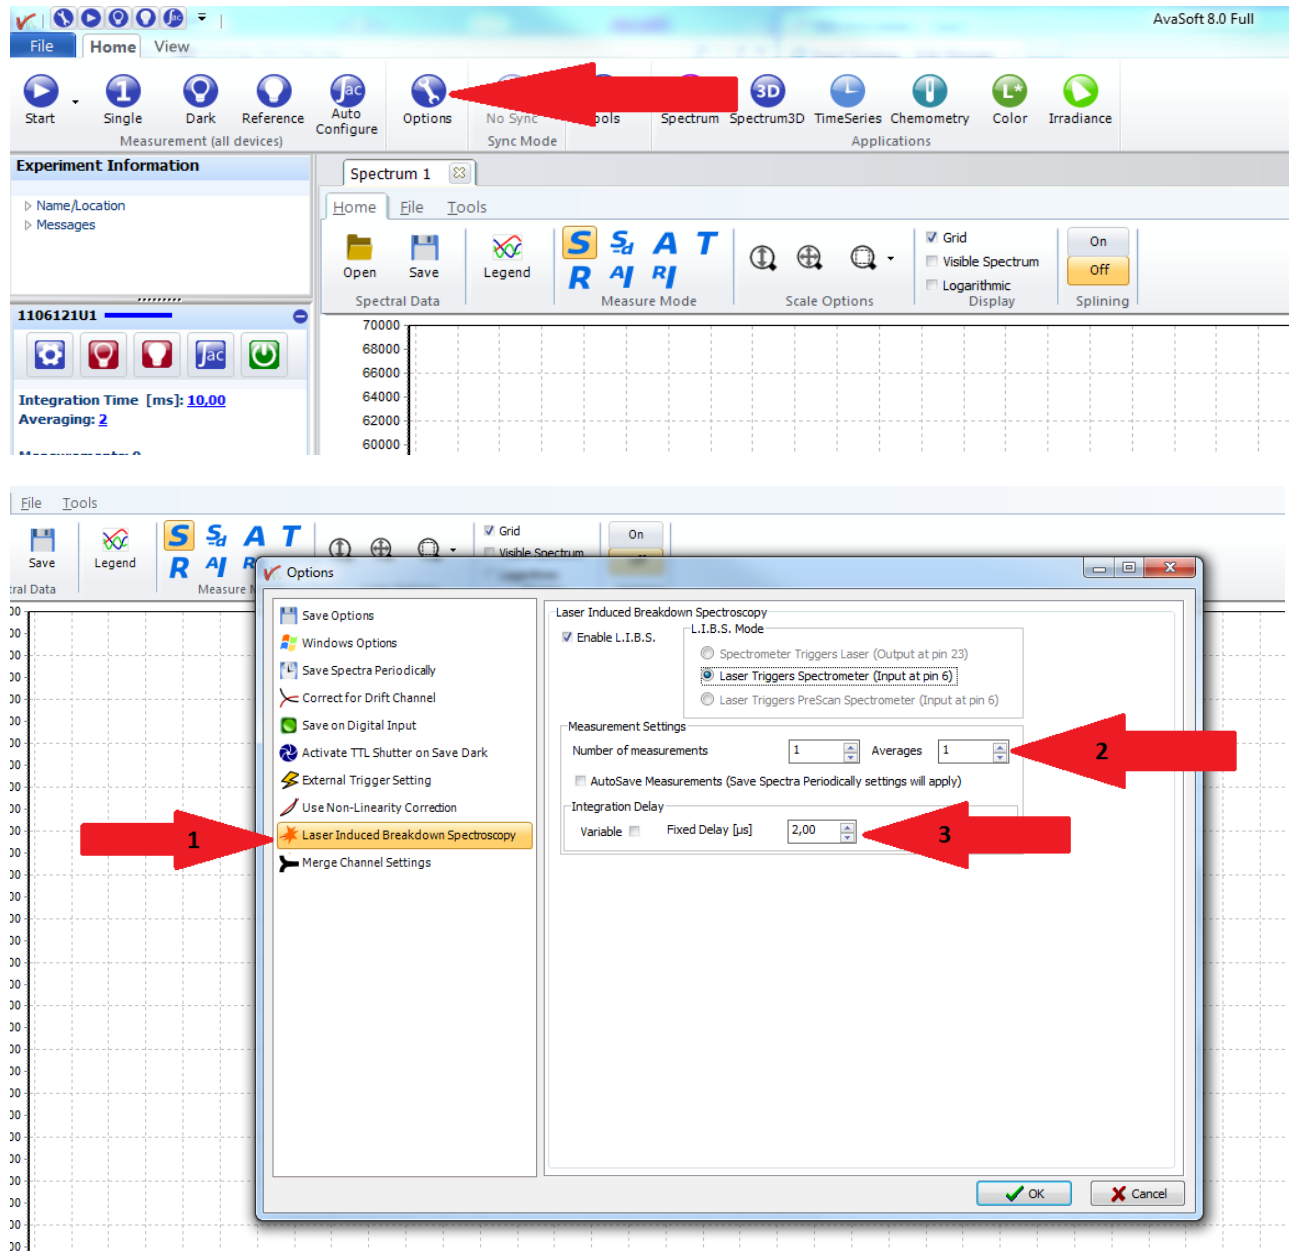

- 1) Please select "Laser Induced Breakdown Spectroscopy"
- 2) Select the number of measurements and the number of averages.
- 3) Select the delay between the laser and the measurement.